


Single Field Analysis

Eye: Left

Name: krishnaveni, p	ID: 1289340	DOB: 1/23/1948
----------------------	-------------	----------------

Central 24-2 Threshold Test

Fixation Monitor: Blindspot	Stimulus: Ill, White	Pupil Diameter: 8.00mm	Test Date: 11/4/2008
Fixation Target: Central	Background: 31.5 asb	Visual Acuity: 0.70	Test Time: 2:10:43 PM
Fixation Losses: 0/17	Strategy: SITA Standard	Rx: +5.25 DS DC X °	Test Duration: 10:05
False Pos Errors: 4%			Age: 60
False Neg Errors: 7%			
Fovea: 33 dB			

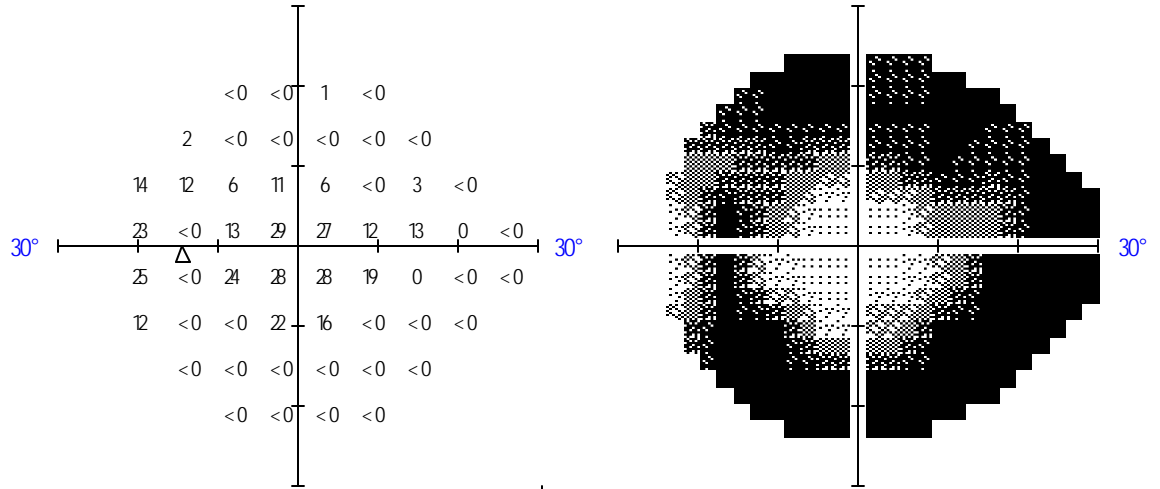


	-28	-29	-25	-29				
	-26	-31	-31	-31	-31	-30		
	-14	-18	-24	-20	-25	-33	-27	-30
	-7	-19	-3	-5	-20	-18	-29	-29
	-5	-7	-4	-4	-13	-31	-31	-29
	-17	-33	-33	-10	-17	-34	-33	-31
	-32	-33	-33	-33	-33	-33	-31	
	-31	-32	-31	-31				

	-21	-22	-18	-22				
	-19	-23	-24	-24	-24	-23		
	-7	-10	-17	-13	-18	-26	-20	-23
	0	-12	4	2	-13	-11	-22	-21
	2	0	3	3	-6	-24	-24	-22
	-10	-25	-26	-3	-9	-27	-26	-24
	-25	-25	-26	-26	-25	-24		
	-24	-24	-24	-24				

GHT: Outside Normal Limits

MD: -23.22 dB P < 0.5%
PSD: 11.03 dB P < 0.5%

Total Deviation

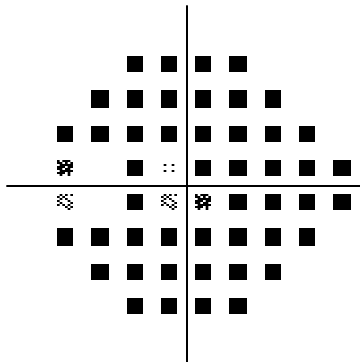

Pattern Deviation

